

ABALATION DEVICE WITH SPIRAL ARRAY ULTRASOUND TRANSDUCER
Yaron Keidar



1/12

FIG. 1A

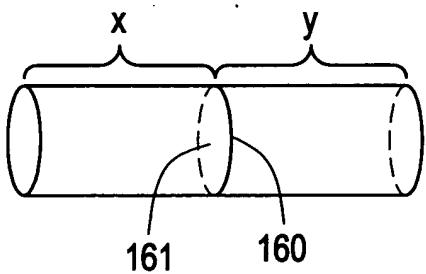


FIG. 1B

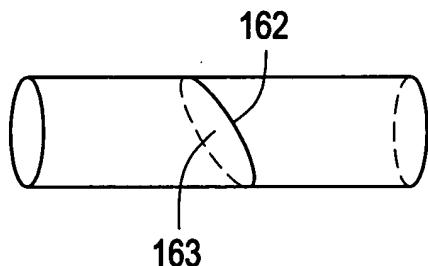


FIG. 1C


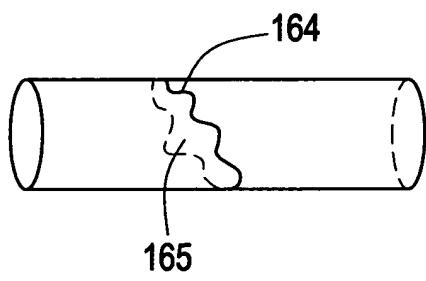



FIG. 1D

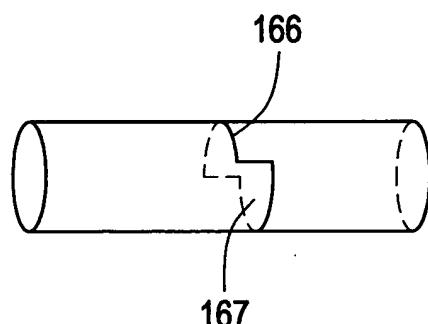

ABALATION DEVICE WITH SPIRAL ARRAY ULTRASOUND TRANSDUCER
Yaron Keidar

2/12

FIG. 2A

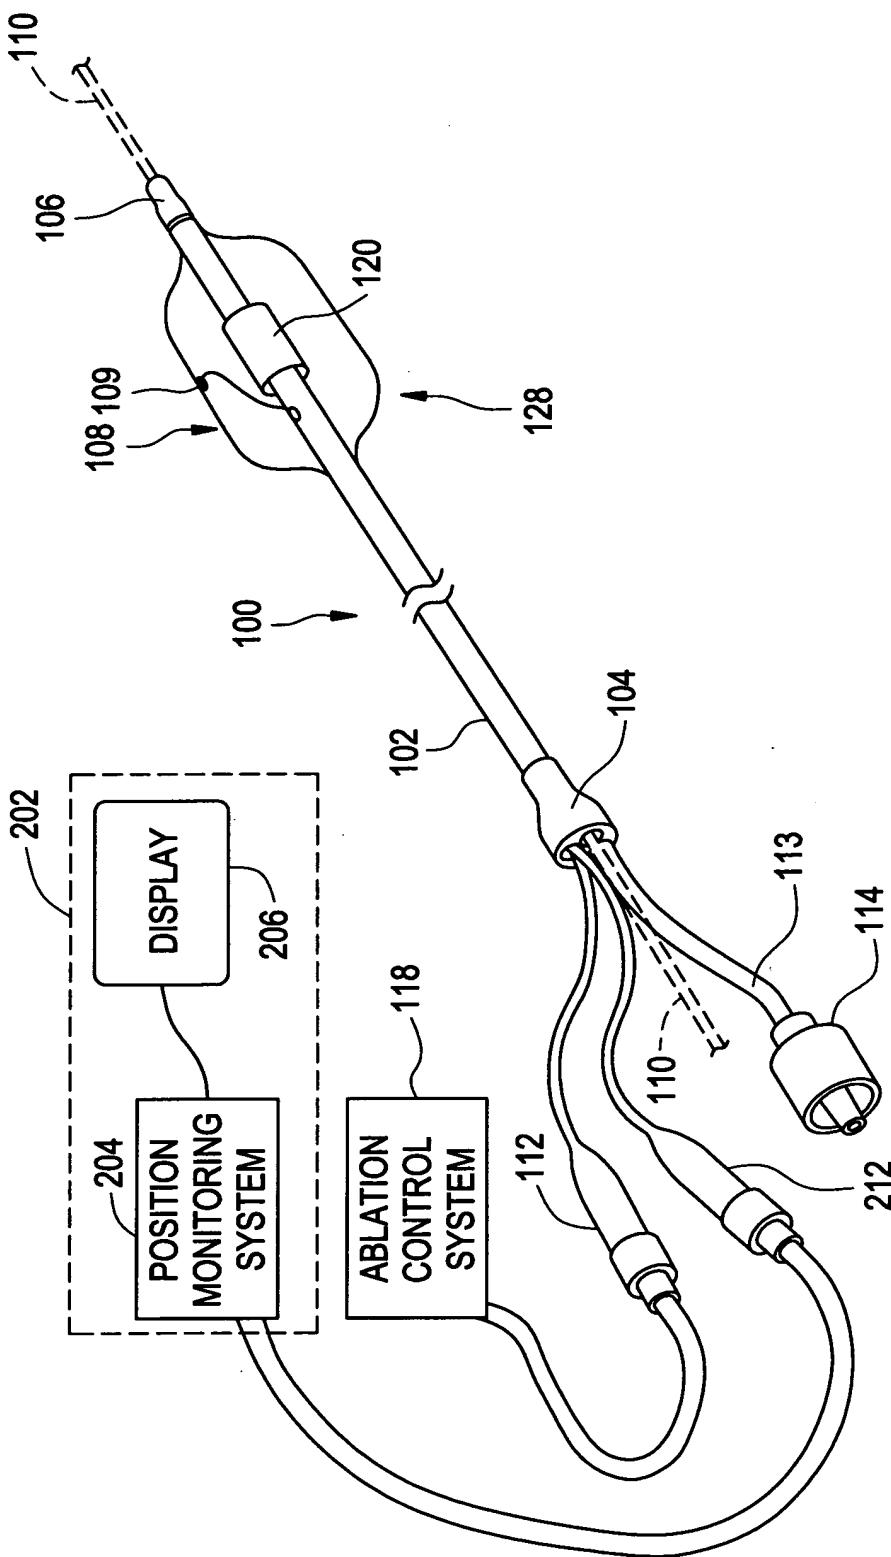

ABLATION DEVICE WITH SPIRAL ARRAY ULTRASOUND TRANSDUCER
Yaron Keidar

3/12

FIG. 2B


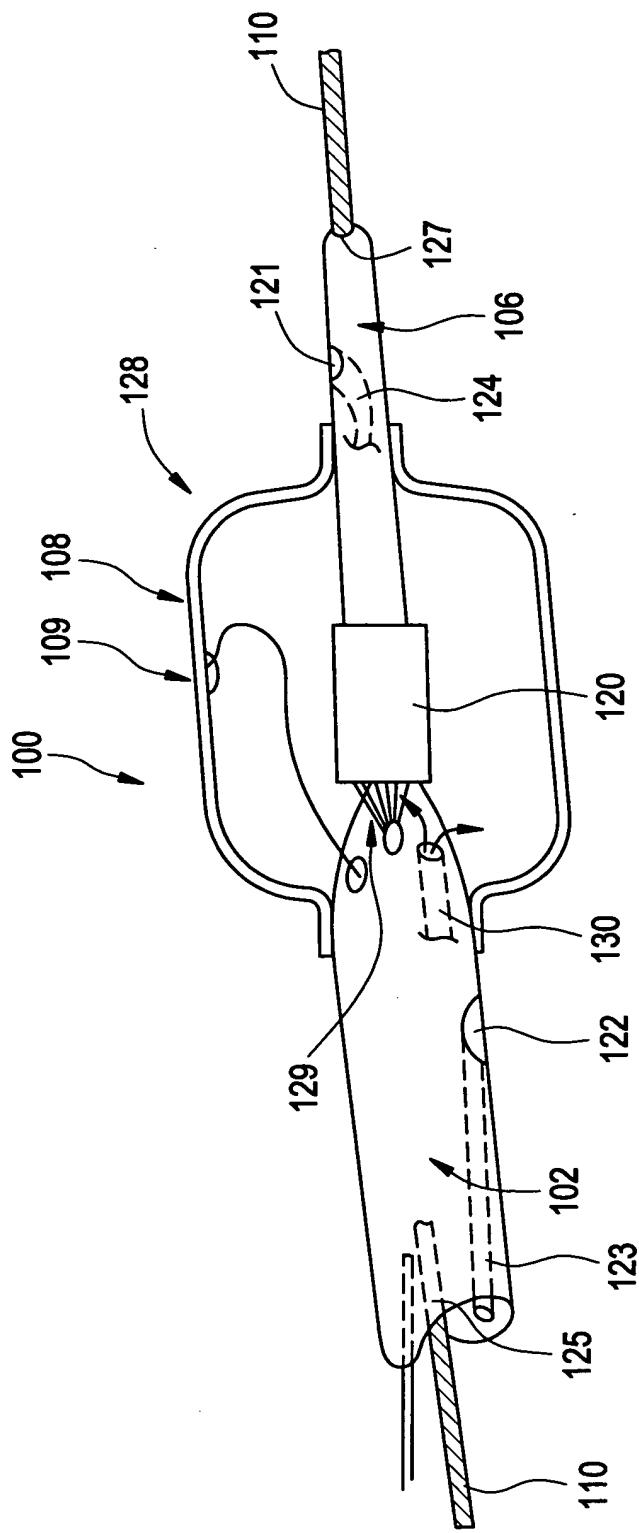


FIG. 3A
PRIOR ART

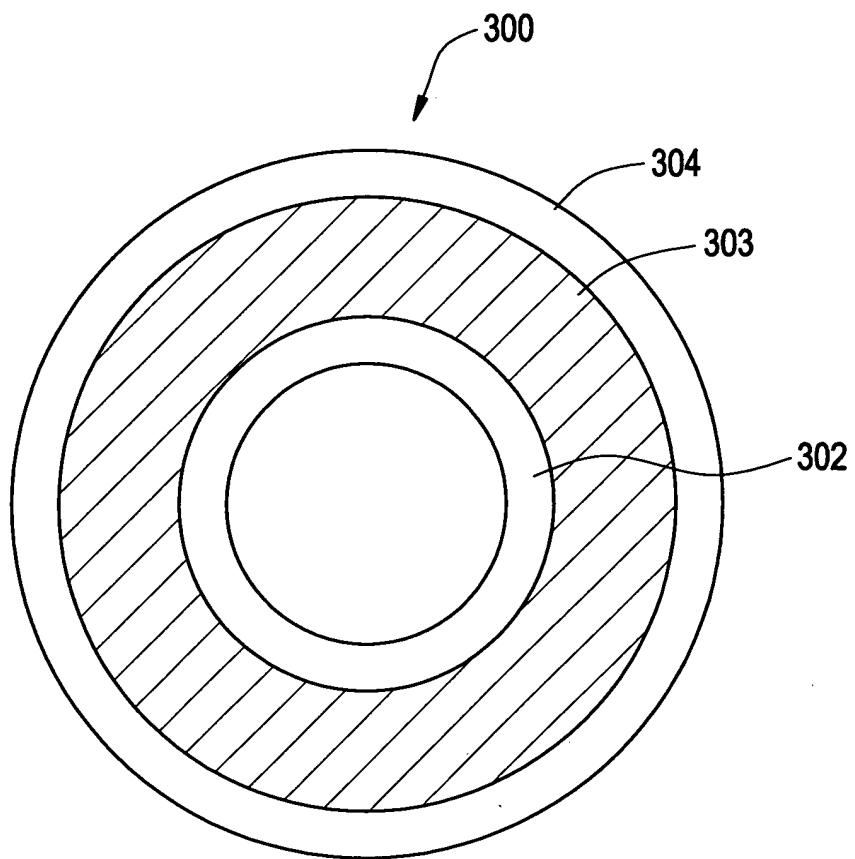

5/12

FIG. 3B
PRIOR ART


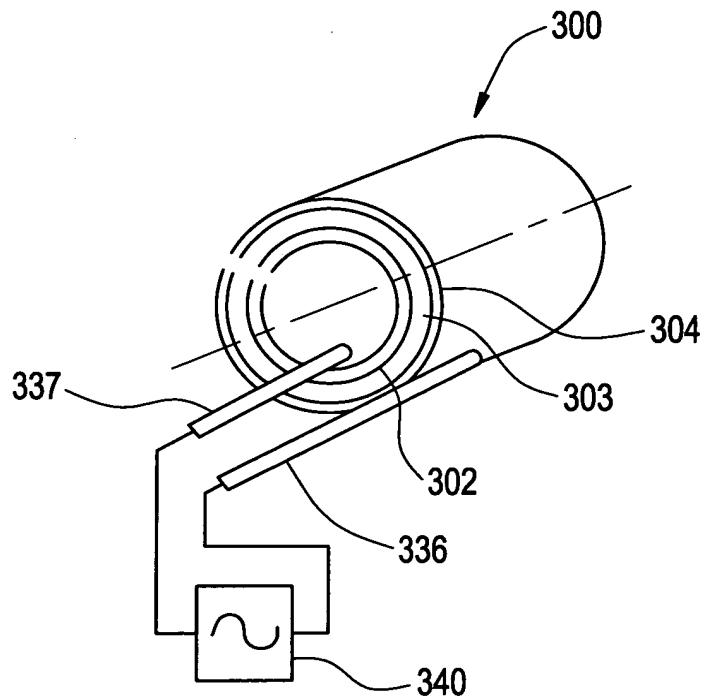


FIG. 3C
PRIOR ART

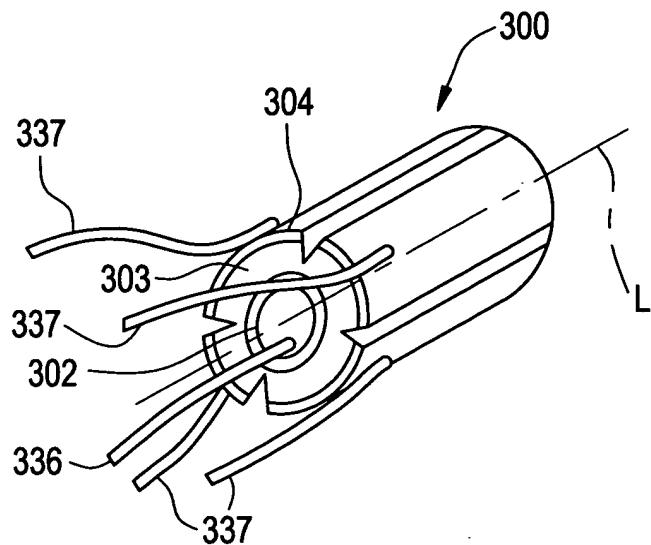

6/12

FIG. 3D
PRIOR ART



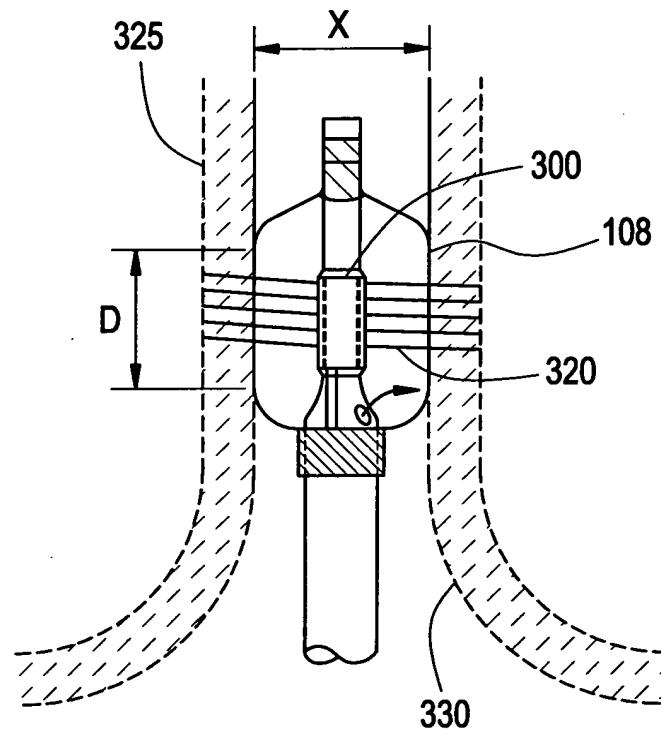


FIG. 3E
PRIOR ART

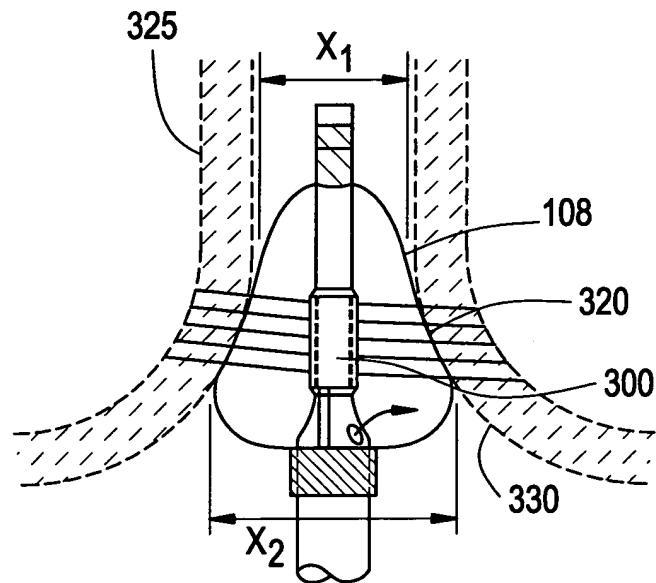

7/12

FIG. 4A

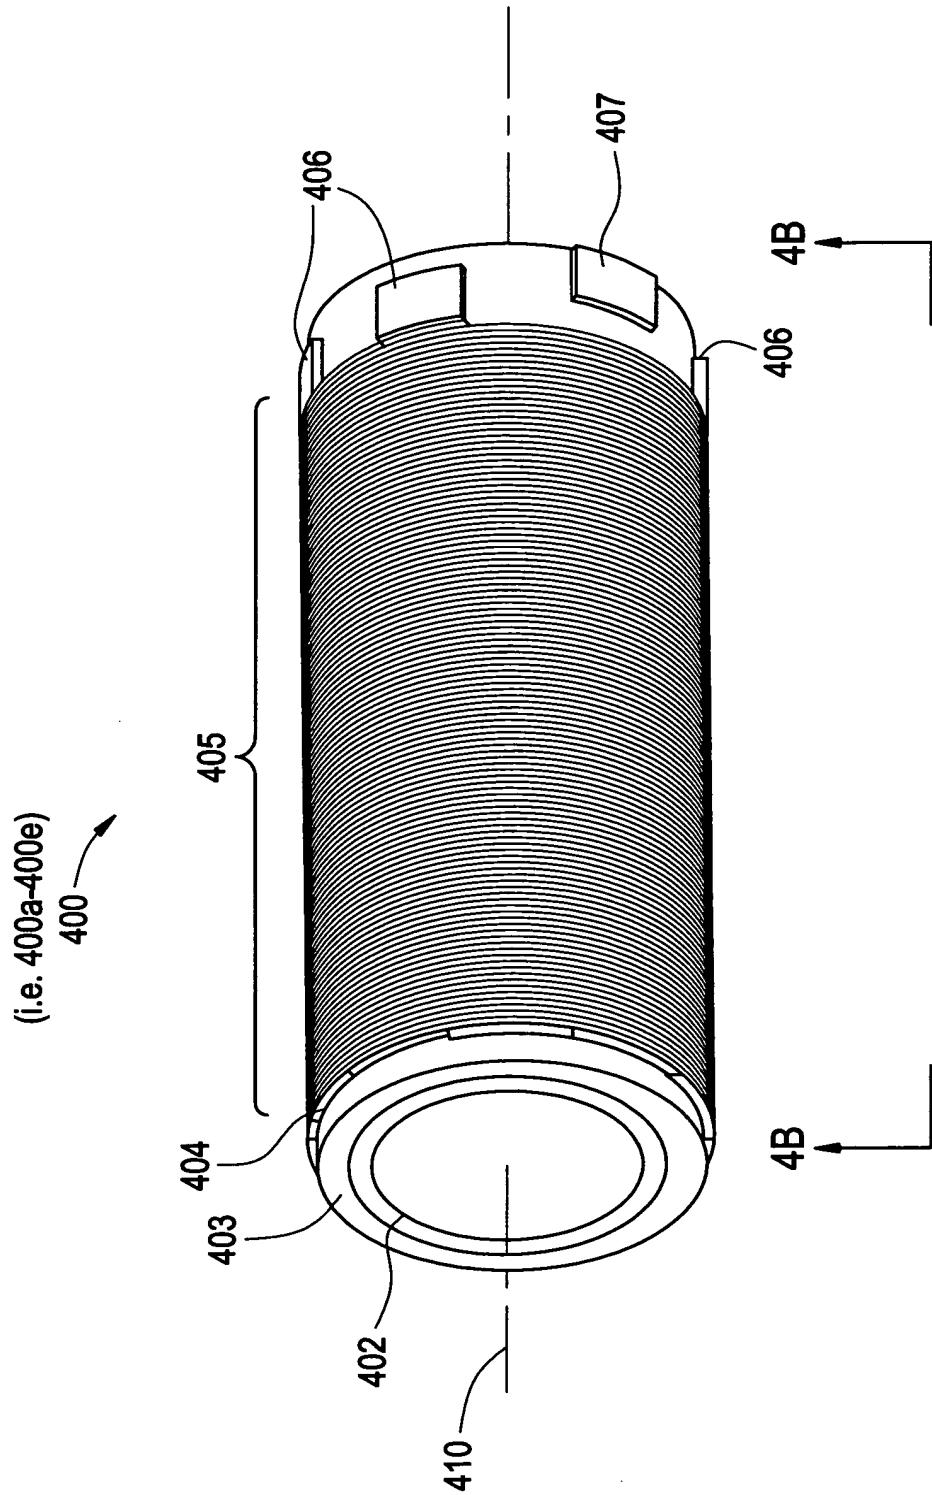

8/12

FIG. 4B

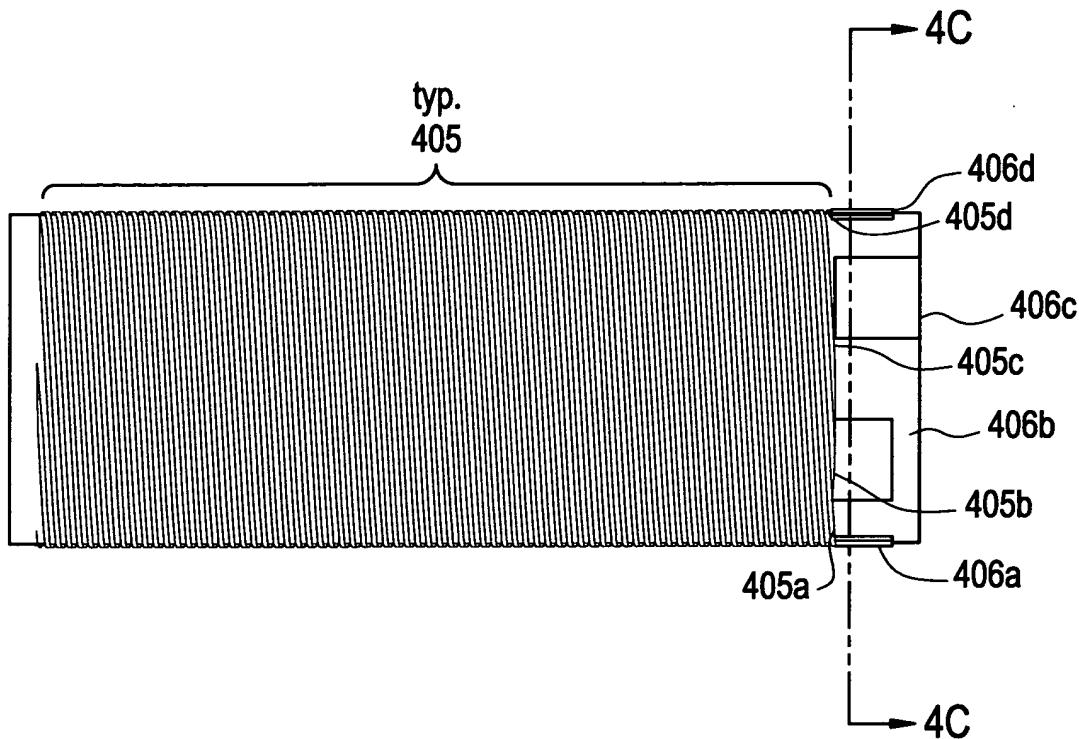


FIG. 4C

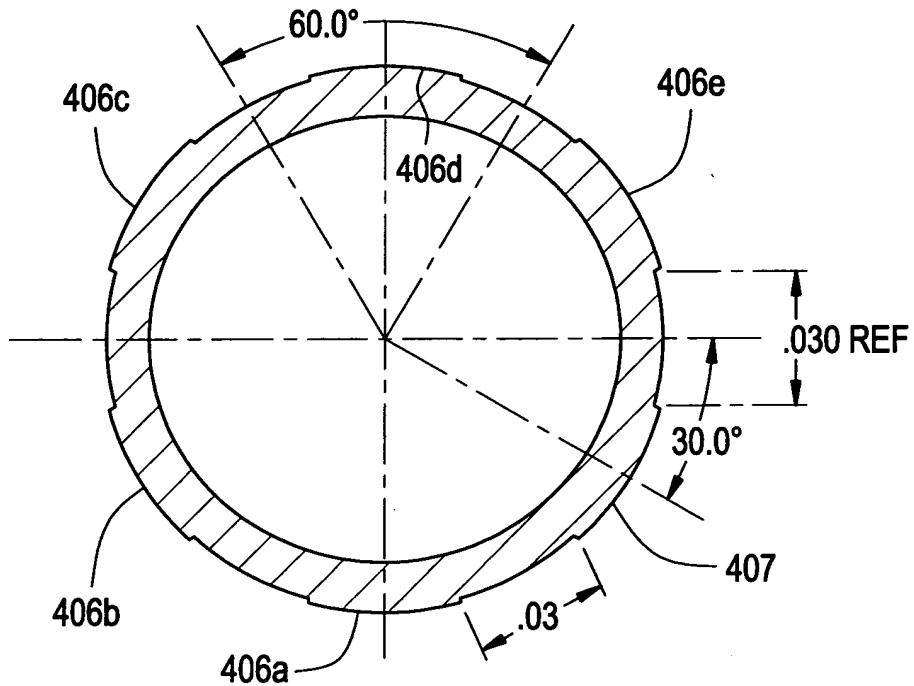


FIG. 5A


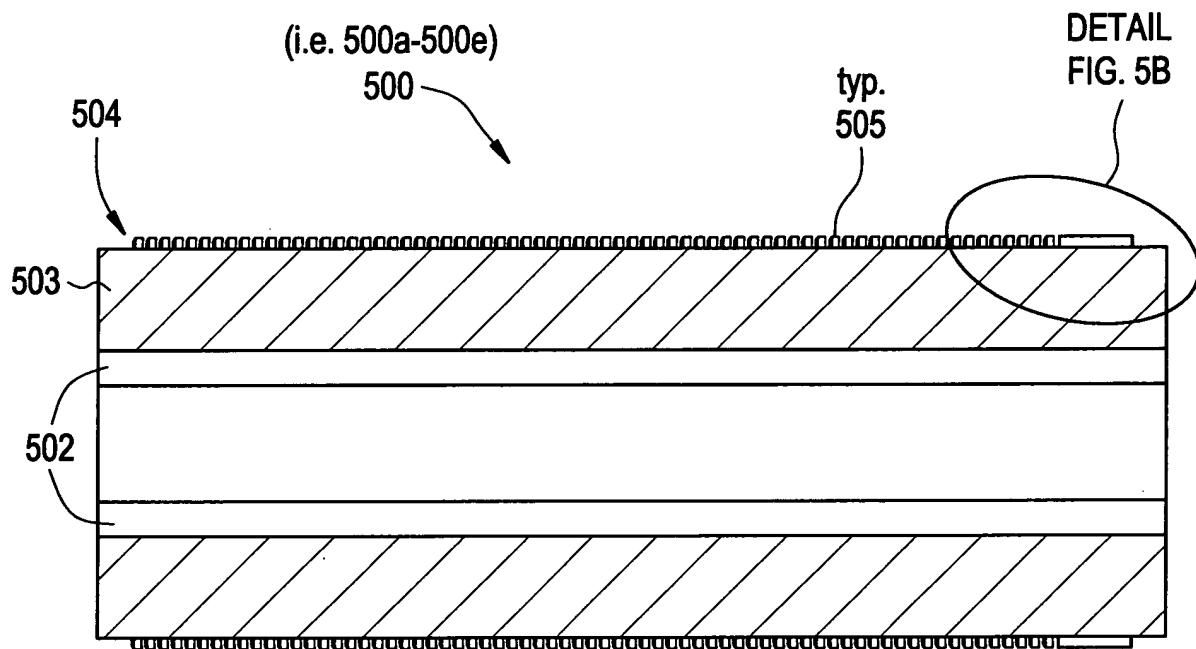


FIG. 5B

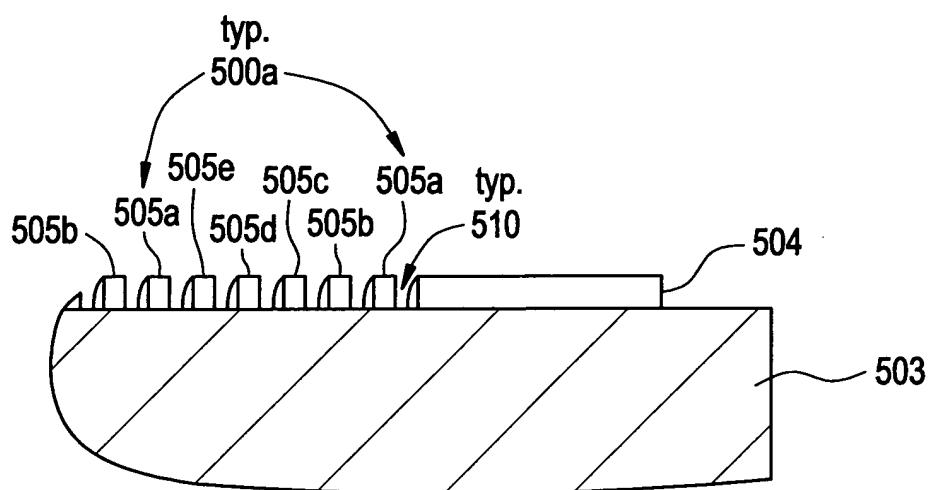

10/12

FIG. 6A


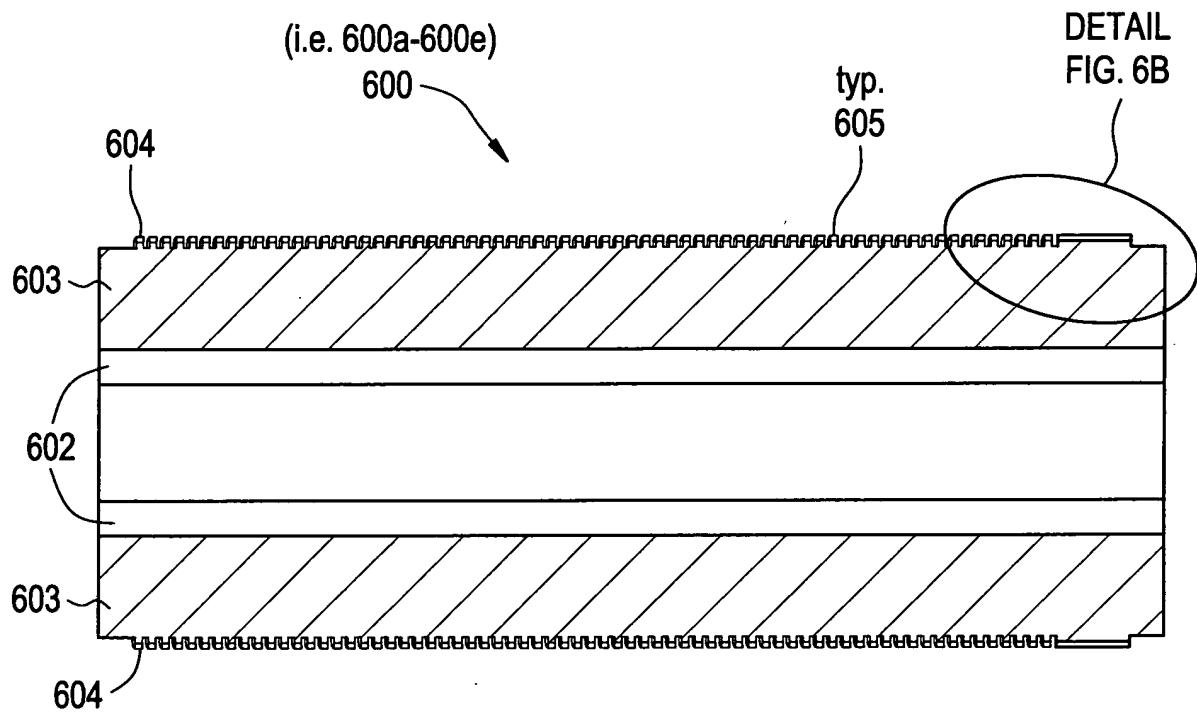


FIG. 6B

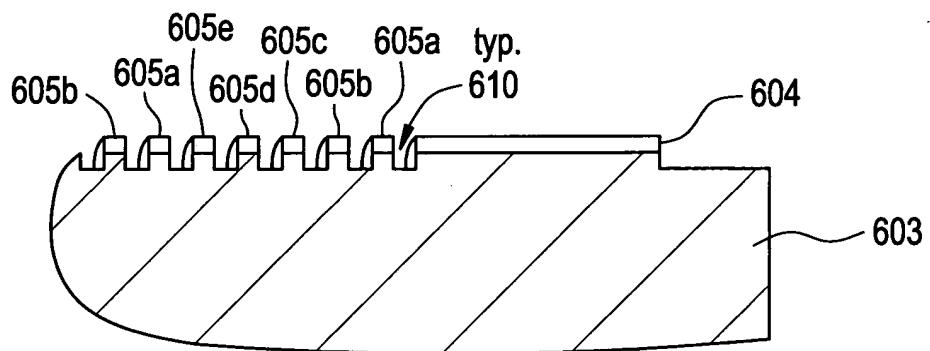

11/12

FIG. 7A


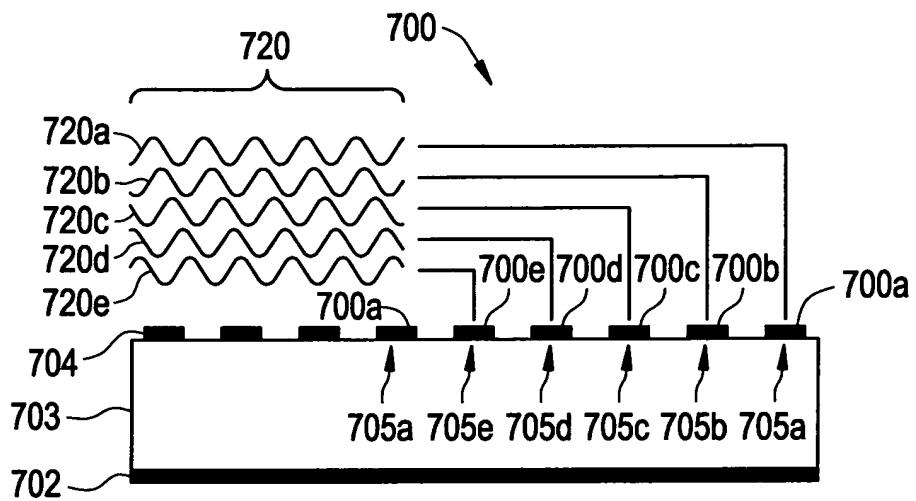


FIG. 7B

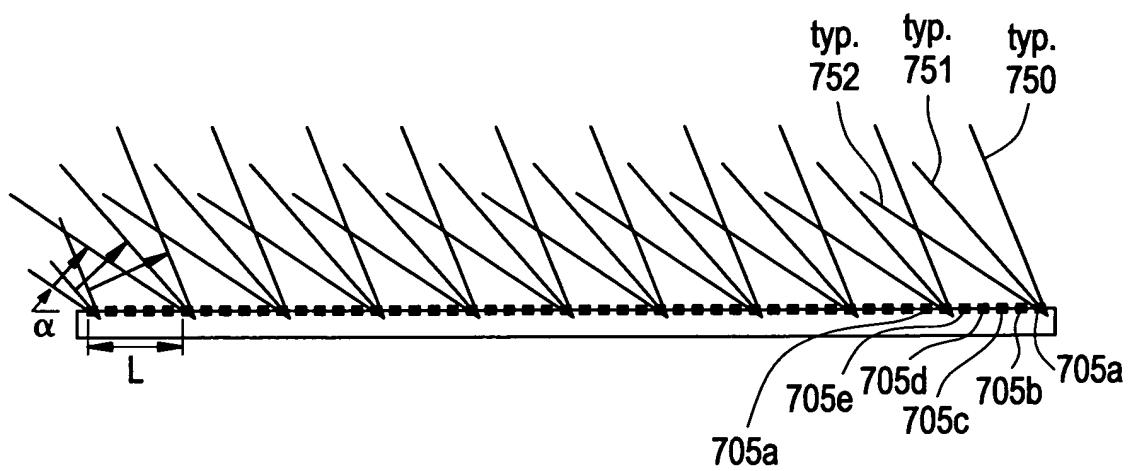

ABLATION DEVICE WITH SPIRAL ARRAY ULTRASOUND TRANSDUCER
Yaron Keidar

12/12

FIG. 7C

